

DICOM

Supplement 188
Multi-Energy CT Imaging

DICOM Working Group 21
Computed Tomography

Short introduction of Multi Energy (ME) Images


Overview:

- Imaging techniques, including scanning, reconstruction, processing, when the scanner utilizes multiple energies from the X-Ray beam spectrum, as opposed to the conventional CT imaging, when a single (accumulated) X-Ray spectrum is used.
- The existing CT and Enhanced CT (eCT) IODs do not adequately describe the new CT multi-energy imaging. Although different vendors apply different scanning and detection techniques to achieve multi-energy images, there is large commonality in the generated diagnostic images.

Goals for ME Image implementation:

- provide new essential ME information (acquisition, reconstruction and processing attributes) within the IOD.
- facilitate fast and easy adoption of standard based ME imaging across the imaging community, both modalities and PACS/Displays.
- address (or at least to minimize) the risk of mis-interpretation when the ME images are displayed by a display does not support the new attributes of the ME-image, including incorrect measurements
- adapt existing attributes of the CT / Enhanced CT IOD to fit ME techniques.


Overview

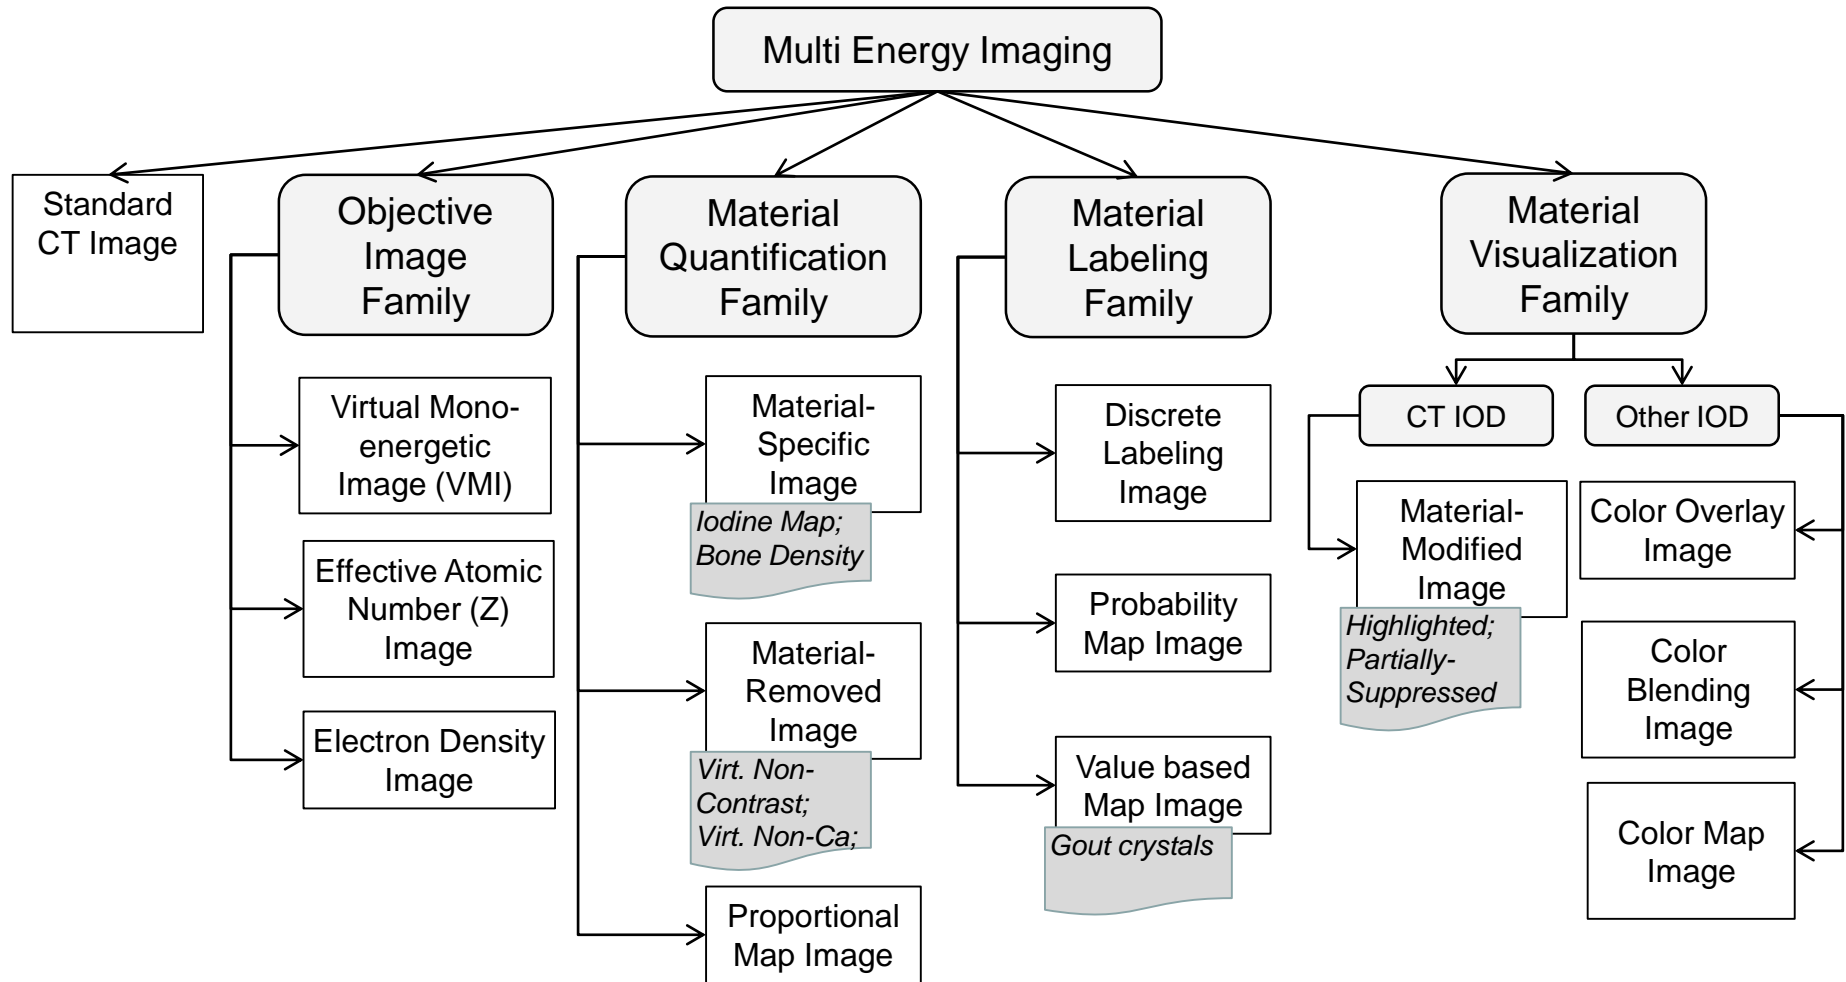

Multi-energy CT Macro (*new added to CT IODs*)

- **Multi-energy Flag (Y/N)**
- **Multi-energy CT Acquisition Sequence (1C, 1 item)**
 - Multi-energy CT Acquisition Sequence (1-N)
 - Multi-Energy Source Technique
 - Multi-Energy Detection Technique
 - *Other ME-specific attributes*
 - Common CT Acquisition Macro
- **Multi-energy CT Processing Sequence (1C, 1 item)**
 - Decomposition Method
 - Decomposition Basis Sequence (2-N items, one for each basis)
 - *Other decomposition attributes*
- **Multi-energy CT Characteristics Sequence (1C)**
 - Monochromatic Energy Equivalent (*for Virtual Monochromatic Image*)
 - Multi-energy Quantification CT Image Macro
 - Specific Material Code Sequence
 - Material Modification Sequence
 - Multi-energy Labeling CT Image Sequence (1 item)
 - Material Labeling Type
 - Material Modification Sequence

Multi-Energy CT Acquisition Techniques

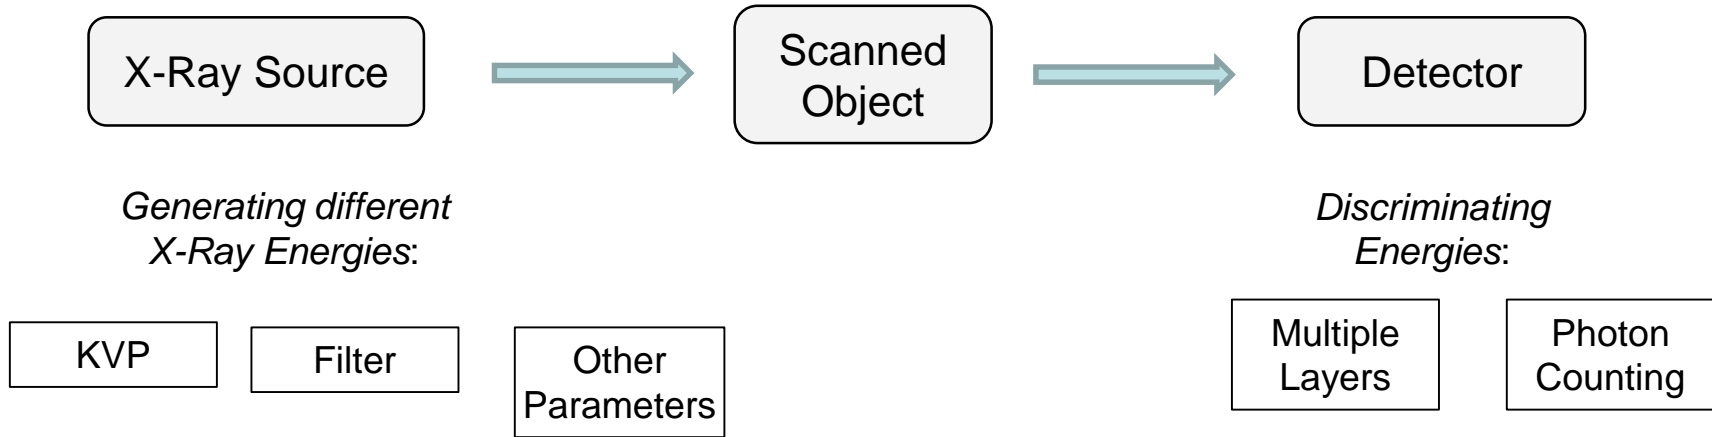

Methods to separate at least two energies include

- Multiple Scans of the same area with diff parameters
- Multiple X-Ray Sources and/or Detectors
- Switch KVP during the rotation
- One source with Multi-Layer Detector
- One source with Photon Counting Detector

“Objective” Images

Data Acquisition

A1

A2

...

An

Decomposition to
Base Components

M1

M2

...

Mn

Generation of
Diagnostic images

Virtual
Monochromatic

Effective
Atomic Number

Electron
Density

*Described in ME CT
Acquisition Sequence*

*Described in ME CT
Processing Sequence*

*Described in ME CT
Characteristics Sequence
(currently just keV for VMI)*

“Material” Images

Data
Acquisition

Decomposition to and/or Classification of
two or more Materials

Generation of
Diagnostic images

A1

A2

...

An

M1

M2

...

Mn

Material
Quantification
Family

Material Labeling
Family



Material
Visualization
Family

*Described in ME CT
Acquisition Sequence*

*Described in ME CT
Processing Sequence*


*Described in ME CT
Characteristics Sequence*

Material Images Generation

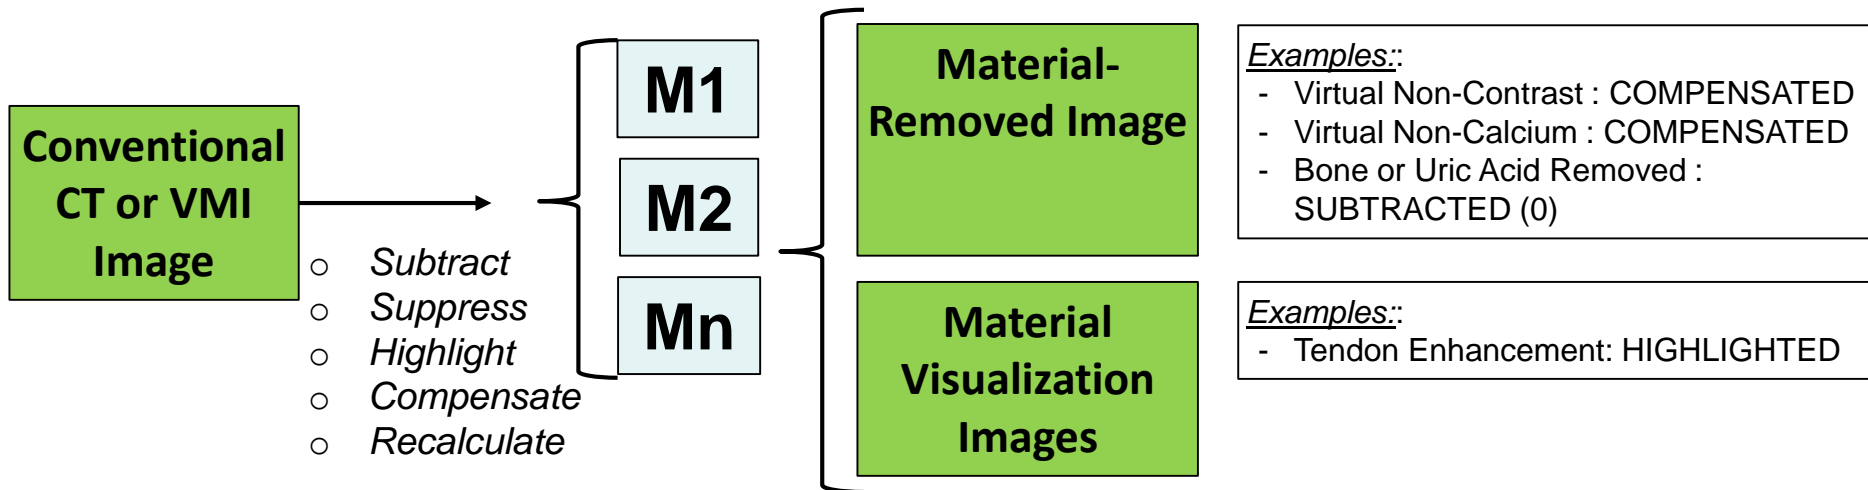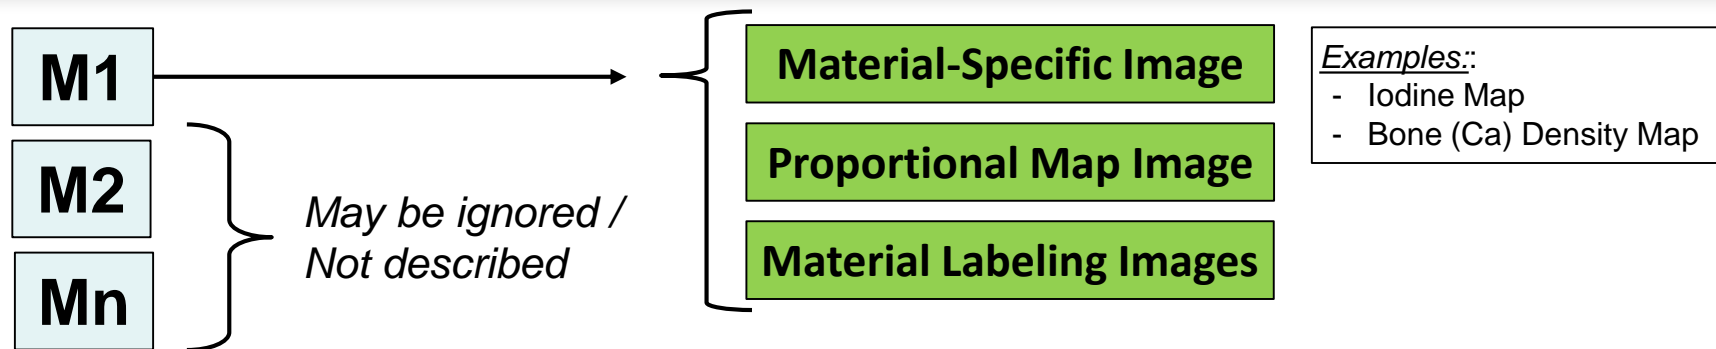


Material Labeling Images


Discrete Labeling (most-probable material):

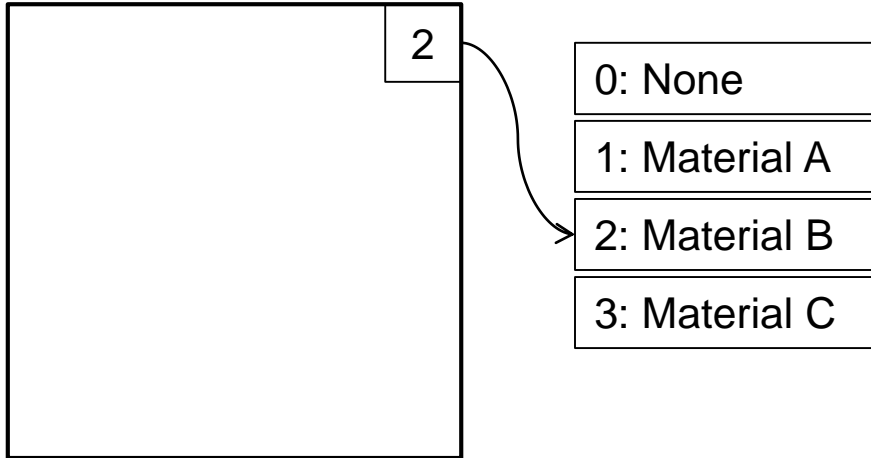


Proportional:

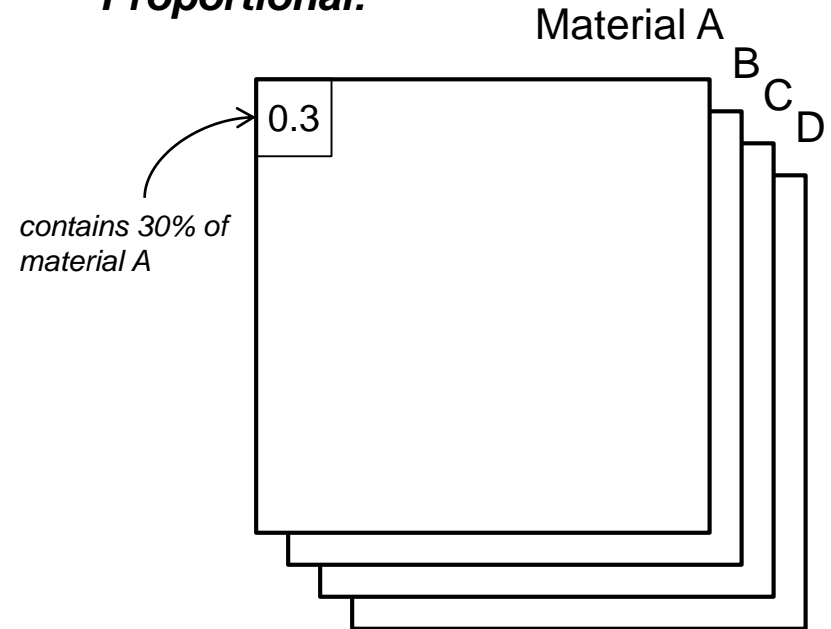

Value based:

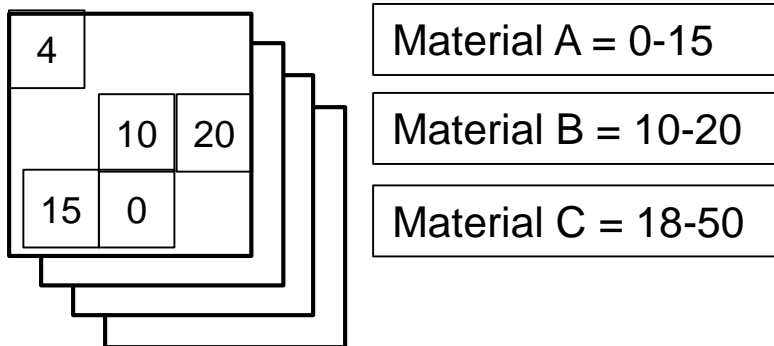


Probability: Material A

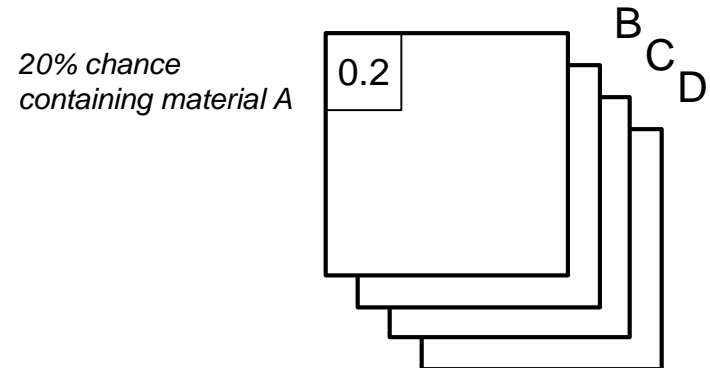

“Visualization” Images

Color Overlay

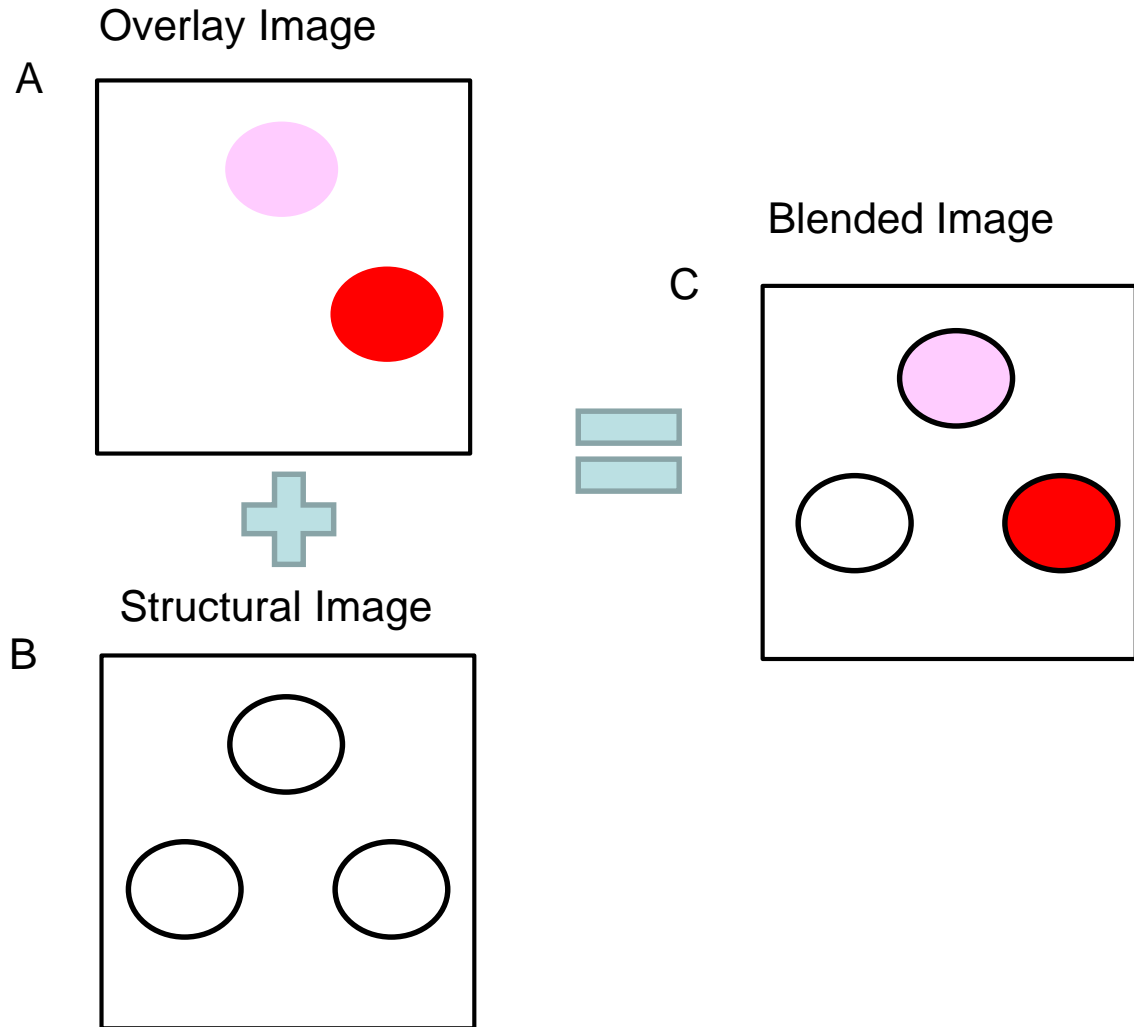

A) A CT image that is windowed to highlight a particular material with a color map applied. It also may have a translucency applied to be able to see the image underneath. (E.g. Iodine image, Effective Z image)

B) A structural image showing the anatomical structure. (E.g. Monochromatic image)

C) The result image (combined information e.g. Secondary Capture, Blending, ...)