

1	Status	Final Text
2	Date of Last Update	2015/03/18
3	Person Assigned	David Clunie
4		mailto:dclunie@dclunie.com
5	Submitter Name	David Clunie
6		mailto:dclunie@dclunie.com
7	Submission Date	2014/07/17

8	Correction Number CP-1424	
9	Log Summary: Remove Information Model figure that applies only to retired Normalized IODs	
10	Name of Standard	
11	PS3.3 2015a	
12	Rationale for Correction:	
13	The DICOM Information Model (as opposed to the Real-World Model) does not contain the Series entity. However, since the IODs	
14	to which the figure applies have been retired, it is appropriate to just remove it, since it serves no purpose.	
15	Correction Wording:	

7 DICOM model of the real-world

Remove Figure 7-2a, the content of which is shown here:

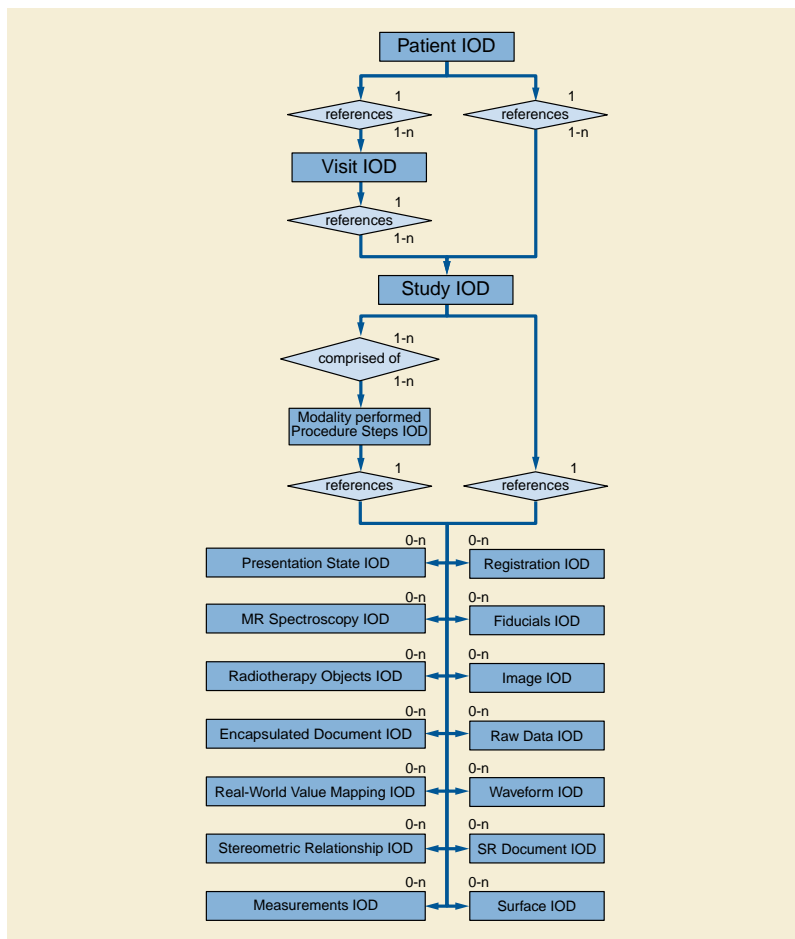


Figure 7-2a. DICOM Information Model

7.1 DICOM Information Model

The DICOM Information Model is derived from the DICOM Model of the Real World. The DICOM Information Model presented by **Figure 7-2a**, Figure 7-2b, Figure 7-2c and Figure 7-2d identify the various IODs specified by this Standard and their relationships. There is not always a one-to-one correspondence between DICOM Information Object Definitions and Real-World Objects. For example a Composite IOD contains Attributes of multiple real-world objects such as series, equipment, frame of reference, study and patient.

The entities in **Figure 7-2a**, Figure 7-2b, Figure 7-2c and Figure 7-2d correspond to IODs defined in Annex A, Annex B and Annex C.