

DICOM Correction Proposal

STATUS	Final Text
Date of Last Update	2018/06/05
Person Assigned	David Clunie
Submitter Name	WG-02, Francisco Sureda (email: francisco.sureda@med.ge.com)
Submission Date	2018/01/22

Correction Number	CP-1768
Log Summary:	Correct PS3.17 Figure FFF.2.3-1
Name of Standard	PS3.17 2018b
Rationale for Correction:	The Figure FFF.2.3-1: "Example of Usage of Photometric Interpretation" of PS3.17 does not reflect the original figure of the Supplement 139 Figure Z.2.3-1.
Correction Wording:	

Change in PS 3.17 2017d: change Figure FFF.2.3-1

The current Figure FFF.2.3-1 of PS3.17 is confusing because it does not show clearly which system (A and B) displays white or black blood vessels when Photometric Interpretation is MONOCHROME1 and 2.

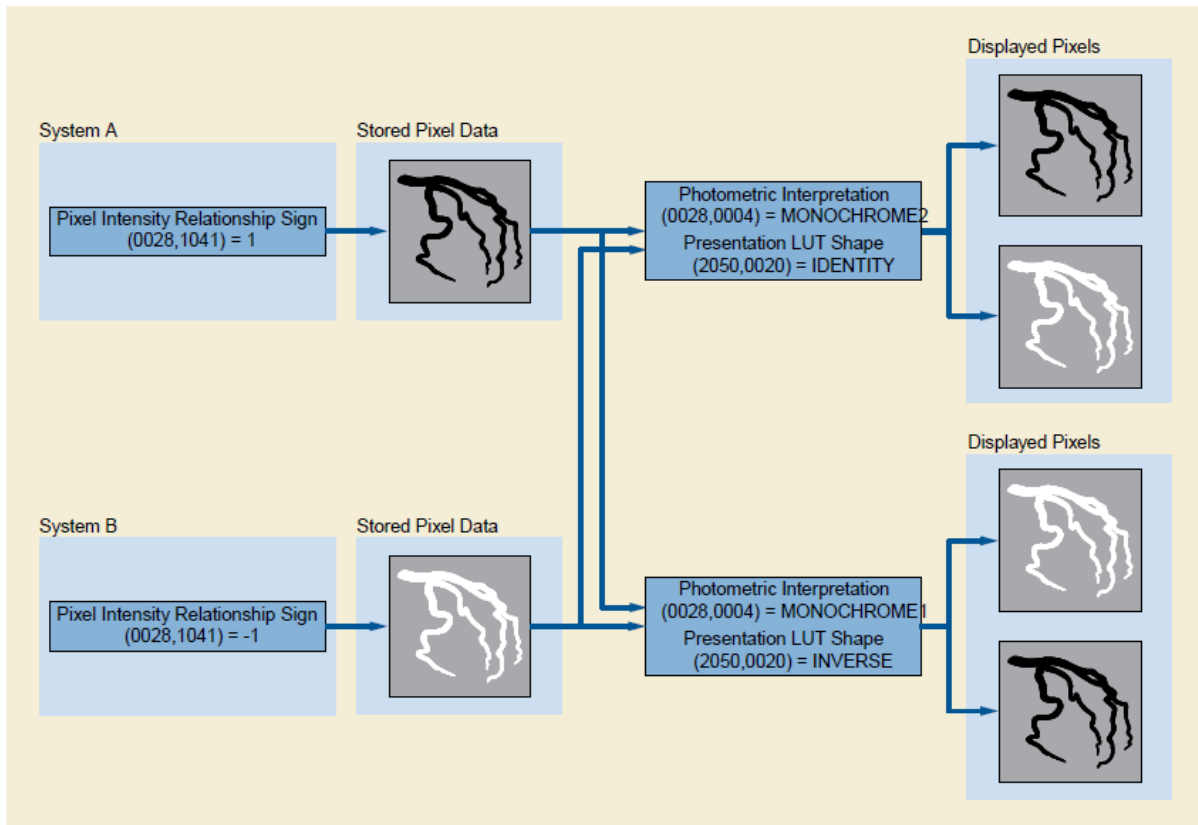


Figure FFF.2.3-1. Example of usage of Photometric Interpretation

Need to change the Figure FFF.2.3-1 to show clearly that:

System A

- displays black blood vessels when Photometric Interpretation is MONOCHROME2
- displays white blood vessels when Photometric Interpretation is MONOCHROME1.

System B

- displays white blood vessels when Photometric Interpretation is MONOCHROME2
- displays black blood vessels when Photometric Interpretation is MONOCHROME1.

as shown in the original figure hereafter of Supplement 139:

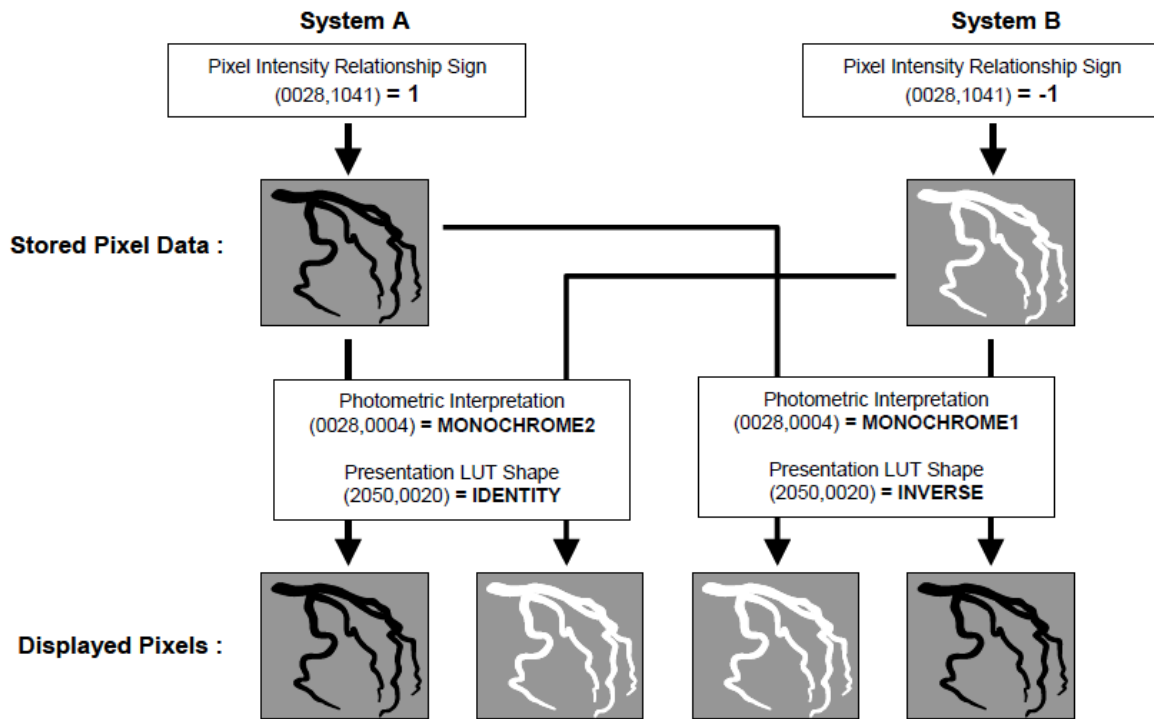


Figure Z.2.3-1
Example of usage of Photometric Interpretation